


# LAP-BAND® System Access Port II Kit

DIRECTIONS FOR USE (DFU)



Access Port Needle



Access Port Priming Needle



Access Port II



End Plug



Band Priming Needle



Stainless Steel Connector



Tubing

Rx Only



# LAP-BAND® System Access Port II Kit

## INTRODUCTION

The LAP-BAND® System Access Port II is connected to the LAP-BAND® Adjustable Gastric Banding System with silicone tubing. The Access Port II is for percutaneous adjustment of the stoma diameter and is self-sealing when penetrated by the Access Port needle. The Access Port II is part of the LAP-BAND® Adjustable Gastric Banding System and is available as a replacement port.



The Access Port II has three variations and are distinguishable via x-ray. The chart below indicates visible differences, fill volumes, and which LAP-BAND® Systems they are used for.

### ACCESS PORT II VARIATIONS

LAP-BAND® System	Septum	#Radiopaque Markers	Fill Volume
9.75 /10.0	white	0	0-4 cc
VG AP® Standard	clear	1	0-10 cc
AP® Large	clear	2	0-14 cc

## DESCRIPTION

The Access Port II Kit contains the following components:



## ACCESS PORT FEATURES:


### Access Port II Kit (9.75/10.0) Access Port II Kit (VG, AP® Standard) Access Port II Kit (AP® Large)

Features Include:


- High-compression septum; tested to over 200 punctures with a 20 gauge non-coring needle.
- Titanium protective base plate; positive tactile feedback, designed for long-term durability when the access port needle makes contact, resists gouging from repeated needle contact for long-term reservoir integrity.
- Radiopaque and compatible with diagnostic imaging; including MRI and CT scanning (the small stainless steel connector attached to the access port tubing has been reported to interfere minimally with MRI scanning).
- Contoured acetal copolymer housing; light-weight, smooth and round
- A stainless steel connector which is used with ligatures to join the tubing of the band to the Access Port II.




Cross-section view of the Access Port II

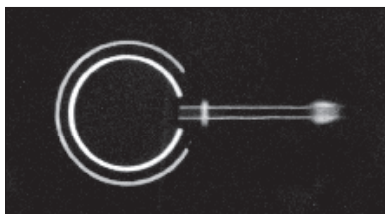

Radiographic top or bottom view of the Access Port II for the LAP-BAND® System 9.75 and 10.0

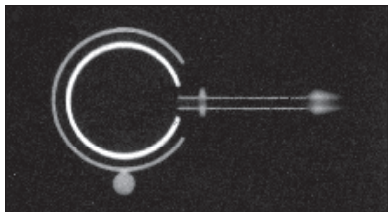

Radiographic top or bottom view of the Access Port II for the LAP-BAND<sup>®</sup> VG System, and the LAP-BAND AP<sup>®</sup> System Standard. Note the single radiopaque marker.

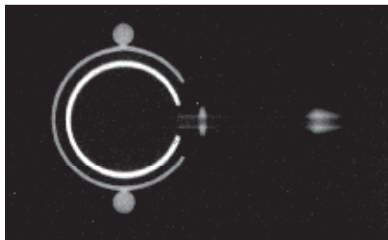

Radiographic top or bottom view of the Access Port II for the LAP-BAND AP<sup>®</sup> System Large. Note the two radiopaque markers.

## INDICATIONS

Indications for Access Port II replacement are:

1. A leaking port (the LAP-BAND<sup>®</sup> System will not maintain its adjustment).
2. Due to removal of an Access Port II from an infected site.
3. Contamination of the Access Port II.

## CONTRAINDICATIONS

The Access Port II is contraindicated in the patients where the LAP-BAND<sup>®</sup> System is contraindicated, and:

1. Patients who have an infection anywhere in the body or where the possibility of contamination prior to or during the surgery exists.
2. Patients who are known to have, or suspected to have, an allergic reaction to materials contained in the system or who have exhibited a pain intolerance to implanted devices.

## WARNINGS AND PRECAUTIONS

Patients should be advised not to consider their implants lifetime devices; explant and replacement surgery may be indicated at any time. Medical management of adverse reactions may include explantation. Revision surgery for explantation and replacement may also be indicated to achieve patient satisfaction.

## COMPLICATIONS

Complications which may result from the use of this product include the risks associated with the medications and methods utilized in the surgical procedure, the risks associated with any surgical procedure and the patient's degree of intolerance to any foreign object implanted in the body.

Infection can occur in the immediate post-operative period or years after insertion of the device. In the presence of infection or contamination, removal of the device is indicated.

Deflation of the band may occur due to leakage from the band, the port, or the connecting tubing.

The material in this device has been shown in biocompatibility studies to cause slight irritation in intramuscular implantation in animal models.

## HOW SUPPLIED

The Access Port II and components are for single use only.

The Access Port II and components are provided sterile in double packaging with a protective outer container. The Access Port needle is provided sterile in separate packaging. If the package has been opened outside the sterile field, the product must be considered non-sterile.

## ACCESS PORT II PREPARATION

1. Remove Access Port along with the 22 gauge blunt flushing needle from the sterile container
2. The blunt flushing needle fits loosely inside the fill tubing of the Access Port. Do not attempt to insert it into the port.
3. Hold the Access Port with the fill tubing in an upright position with the port on the bottom.
4. Attach a 5cc saline-filled syringe to the blunt flushing needle.
5. Inject sterile saline to irrigate the Access Port. As it fills, all air and excess fluid will be forced out of the tubing past the blunt flushing needle.
6. Keep the port tubing upright until it is attached to the band fill tubing.
7. The Access Port and tubing are now full of saline, mostly free of air, and ready to be attached to the implanted band tubing.

## RETURNED GOODS POLICY

Authorization must be received from your distributor prior to return of the merchandise. Merchandise returned must have all the manufacturer's seals intact to be eligible for credit or replacement. Products returned may be subject to restocking charges.

## **LIMITED WARRANTY, LIMITATION OF LIABILITY AND DISCLAIMER OF OTHER WARRANTIES.**

There is no express or implied warranty, including without limitation any implied warranty of merchantability or fitness for a particular purpose, on the Apollo Endosurgery, Inc. product(s) described in this publication. To the fullest extent permitted by applicable law, Apollo Endosurgery, Inc. disclaims all liability for any indirect, special, incidental, or consequential damages, regardless of whether such liability is based on contract, tort, negligence, strict liability, products liability or otherwise. The sole and entire maximum liability of Apollo Endosurgery, Inc., for any reason, and buyer's sole and exclusive remedy for any cause whatsoever, shall be limited to the amount paid by the customer for the particular items purchased. No person has the authority to bind Apollo Endosurgery, Inc. to any representation or warranty except as specifically set forth herein. Descriptions or specifications in Apollo Endosurgery, Inc. printed matter, including this publication, are meant solely to generally describe the product at the time of manufacture and do not constitute any express warranties or recommendations for use of the product in specific circumstances. Apollo Endosurgery, Inc. expressly disclaims any and all liability, including all liability for any direct, indirect, special, incidental, or consequential damages, resulting from reuse of the product.

## **AUTHORIZED TRAINING PROGRAM AND PRODUCT INFORMATION**

LAP-BAND® System placement is an advanced laparoscopic procedure. Surgeons planning LAP-BAND® System placement must participate in a LAP-BAND® System training program authorized by Apollo Endosurgery, Inc. or an authorized Apollo Endosurgery, Inc. distributor. This required training program is specific to the Apollo Endosurgery, Inc. LAP-BAND® System and does not qualify for use with other gastric bands.









For additional information please contact:

Manufacturer  
Apollo Endosurgery, Inc.  
Austin, TX 78746, U.S.A.  
Tel: (512) 279-5100  
Fax: (512) 279-5105

**CAUTION:** This device restricted to sale by or on the order of a physician.

Not made with natural rubber latex.

Patented. See: [www.apolloendo.com/patents](http://www.apolloendo.com/patents)

	<p>Sterilized using steam or dry heat.</p>
	<p>Caution. See Instructions for Use.</p>
	<p>Single Use Only. Do Not Re-use.</p>
 <p>YYYY-MM-DD</p>	<p>Use By Year, Month, &amp; Day</p>
	<p>Manufacturer</p>
	<p>Serial Number</p>
	<p>Reference Number</p>
	<p>Do not use if package is damaged</p>
<p><b>Rx Only</b></p>	<p>Caution: Federal law (USA) restricts this device to sale by or on the order of a physician.</p>



Manufacturer  
Apollo Endosurgery, Inc.  
Austin, TX 78746 U.S.A.

Assembled in Costa Rica

Tel: (512) 279-5100  
Fax: (512) 279-5105

[www.apolloendo.com](http://www.apolloendo.com)

GRF-00298-00R02

All rights reserved.

© 2014 Apollo Endosurgery, Inc., Austin, TX

Apollo Endosurgery, LAP-BAND, and LAP-BAND AP  
are worldwide trademarks or registered trademarks  
of Apollo Endosurgery, Inc.